

# The effect of magnesium and copper addition on the microstructure, mechanical properties, and corrosion rate of as-cast biodegradable zinc alloys

Magdalena GIELECIAK<sup>1</sup> \*, Karol JANUS<sup>1,2</sup>, Łukasz MAJ<sup>1</sup>, Paweł PETRZAK<sup>1</sup>,  
Magdalena BIEDA<sup>1</sup>, and Anna JARZEBSKA<sup>1</sup> \*

<sup>1</sup> Institute of Metallurgy and Materials Science, Polish Academy of Sciences, Krakow, Poland

<sup>2</sup> Faculty of Foundry Engineering, AGH University of Science and Technology, Krakow, Poland

**Abstract.** Microstructure, mechanical, and corrosion properties of as-cast pure zinc and its binary and ternary alloys with magnesium (Mg), and copper (Cu) additions were investigated. Analysis of microstructure conducted by scanning electron microscopy revealed that alloying additives contributed to decreasing average grain size compared to pure zinc. Corrosion rate was calculated based on immersion and potentiodynamic tests and its value was lower for materials with Cu content. Moreover, it was shown that the intermetallic phase, formed as a result of Mg addition, constitutes a specific place for corrosion. It was observed that a different type of strengthening was obtained depending on the additive used. The presence of the second phase with Mg improved the tensile strength of the Zn-based materials, while Cu dissolved in the solution had a positive effect on their elongation.

**Keywords:** biodegradable zinc alloys; alloying additives; mechanical properties; microstructure; corrosion rate.

## 1. INTRODUCTION

Recently, zinc has gained popularity in the context of medical applications for temporary biodegradable implants [1–5]. The fact that zinc is an essential element for the human body, responsible for several biological functions such as cell proliferation or apoptosis regulation further increases this attention [6, 7]. What is more, pure zinc has an optimal degradation rate in terms of use as a potential material for biodegradable cardiovascular stents, compared to magnesium (which corrodes too quickly) and iron (which corrodes too slowly) [7]. However, such use is prevented by the low mechanical properties of pure zinc. Overcoming the limitation is possible thanks to zinc-based alloys with magnesium, copper, calcium, silver, or other biocompatible elements [8]. Even small amounts such as 0.1 wt.% of Mg improve the strength of pure zinc almost threefold, reaching the ultimate tensile strength (UTS) of 81.5 MPa. A further increase of Mg content up to 0.8 wt.% results in a constant increase of yield strength (YS) and UTS, reaching 112 MPa and 120 MPa, respectively [9]. Such an improvement is associated with grain boundary strengthening since 0.1 wt.% of magnesium addition led to grain refinement from  $3094 \pm 84 \mu\text{m}$  (for pure Zn) to  $160 \pm 22 \mu\text{m}$ . Further increase of Mg had a beneficial effect on grain size reduction, and, fi-

nally,  $65 \pm 9 \mu\text{m}$  for 0.8 wt.% was obtained [9]. Based on the literature reports, it seems that the threshold for Mg content is 2%. Above this value, the deterioration of properties can be observed. For example, addition of 1 wt.% of Mg [3] caused growth of YS and UTS to about 100 MPa and 150 MPa, 1.2 wt.% [10] to  $116.5 \pm 1.2 \text{ MPa}$ ,  $129.6 \pm 6.4 \text{ MPa}$ , 1.6 wt.% [11] to UTS  $172 \pm 12 \text{ MPa}$ , while a 3 wt.% decrease of YS and UTS to  $65 \pm 9 \text{ MPa}$  and  $84 \pm 9 \text{ MPa}$  [12], respectively, were achieved. While it is known that Mg can strengthen the Zn-based alloy, it has no positive effect on the elongation (A) of the alloys, as with the addition of up to 0.8 wt.% the elongation stayed below 1%. Moreover, when studying its effect on corrosion rate no linear trend indicates that increasing the amount of Mg improves or weakens corrosion resistance [13]. One report [14] focusing on other as-cast binary zinc alloys indicates that copper addition up to 4 wt.% did not significantly affect grain refinement and elongation but did improve UTS from 9.5 MPa for pure zinc to 105.4 MPa for Zn-4Cu. Immersion testing in HBSS performed over periods of five to 40 days revealed better corrosion resistance over a longer time for all investigated Zn-xCu alloys. Combining several alloying additives and creating ternary alloys may bring positive effects in terms of mechanical properties and corrosion rates, both of which are important factors for the potential application of zinc alloys as temporary implants. Zn-Mg-Sr alloys [15] with YS and UTS  $129.08 \pm 5.07 \text{ MPa}$  and  $144.15 \pm 14.97 \text{ MPa}$ , respectively, are an example of this. Manganese addition to Zn-Mg alloy [2] can also increase YS and UTS, yet at the expense of elongation. Moreover, that alloy ex-

\*e-mail: [m.gieleciak@imim.pl](mailto:m.gieleciak@imim.pl), [a.jarzebska@imim.pl](mailto:a.jarzebska@imim.pl)

Manuscript submitted 2023-12-29, revised 2023-12-29, initially accepted for publication 2024-01-21, published in May 2024.

hibits significantly higher corrosion resistance compared to pure Zn. Attempts were also made to create biodegradable ternary alloys with Ti [16] and Ca [17] additions in Zn-Cu and Zn-Mg, respectively. Micro-alloying (0.05 wt.%) of titanium led to improved mechanical properties, but a greater amount (0.1 wt.%) worsened these parameters. Moreover, the corrosion rate increased due to Ti addition. For Zn-1.5Mg-0.1Ca, YS, UTS, and A improvements reaching  $173.8 \pm 15.1$  MPa,  $241.4 \pm 0.4$  MPa, and  $1.72 \pm 0.01\%$ , respectively, were achieved. Therefore, it seems that three-component alloys bring better results in the as-cast state than binary materials. However, selecting the appropriate elements, which will contribute to increased strength and elongation while maintaining the optimal degradation rate of pure Zn still requires investigation.

Thus, the main aim of this work is to design a Zn-Mg-Cu ternary alloy and indicate the effect of magnesium and copper addition on the mechanical and corrosion properties in an as-cast state. The proposed systematic comparison of pure Zn with binary Zn-Mg and Zn-Cu, and finally ternary Zn-Mg-Cu alloy in an as-cast state, will contribute to a better understanding of the effect of particular elements on the microstructure and properties of Zn-based alloys, and thus to the more efficient creation of new materials for medical use as temporary implants.

## 2. MATERIALS AND METHOD

Pure zinc and its alloys, with 1 wt.% of copper, 0.8 wt.% of magnesium, and 0.8 wt.% of magnesium and 0.2 wt.% of copper (denoted as Zn, ZnCu, ZnMg, and ZnMgCu, respectively) were used for the investigation. Zinc (purity of 99.99%), magnesium (purity of 99.99%), and CuZn40 brass were gravity cast in an argon atmosphere at  $650^\circ\text{C}$ . As a result, ingots with 75 mm diameter and 200 mm height were obtained. Microstructural characterization was done with an FEI E-SEM XL30 scanning electron microscope equipped with an energy dispersive spectrometer (EDS) EDAX Genesis. Samples were ground using abrasive papers from 220 to 7000 grit, polished by  $1\ \mu\text{m}$  and  $\frac{1}{4}\ \mu\text{m}$  diamond suspensions, and electropolished with C1 electrolyte under the following conditions: voltage 25 V and time 15 seconds. Additionally, Zn and ZnCu were etched with a 4% nital solution to reveal microstructural features. ImageJ software was used for further microstructural characterization. To confirm the phase composition, X-ray diffraction (XRD) was performed by using Bruker D8 Discover. Corrosion properties were tested by electrochemical and immersion tests. Cubic samples with an area exposed to Hanks' Balanced Salt Solution (HBSS) of  $0.29$  and  $1.7\ \text{cm}^2$ , respectively, for electrochemical and immersion tests were prepared on abrasive papers up to 7000. Potentiodynamic curves were recorded with the use of an Autolab PGSTAT 302 potentiostat and Nova 2.1.4 software. Three measurements were taken for each material, and the average corrosion rate was calculated according to ASTM G31-72. Static immersion tests (IT) were conducted for 24 and 120 hours in HBSS. For this test, four cubic samples from each material were immersed separately in 50 ml of HBSS, in sterile containers that were placed in an incubator at  $37^\circ\text{C}$ . After every 48 h, the corrosion medium was

changed to maintain the pH at 7.4. After the immersion test, the samples were weighed with corrosion products, and then cleaned in ammonium chloride heated to  $70^\circ\text{C}$  for 20 minutes and five minutes in ethanol to remove the corrosion products and weighed again. Based on this, the corrosion rate was calculated according to ASTM G102-89. Mechanical properties were designated by static tensile test on the Instron 6025 modified by a Zwick Roell machine at room temperature ( $22^\circ\text{C}$ ). Three samples of each material with 3 mm diameter and 14 mm gauge length (Fig. 1) were tested at a strain rate of  $10^{-3}\ \text{s}^{-1}$ .

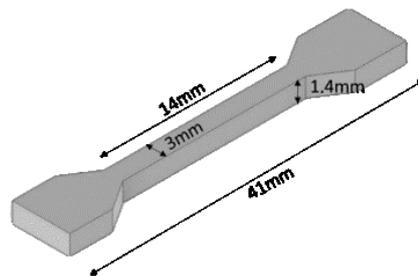


Fig. 1. Example of the specimen used for static tensile test

## 3. RESULTS

### 3.1. Microstructural characterization

Microstructure images obtained by scanning electron microscope are presented in Fig. 2. Pure zinc was characterized by large, equiaxed  $\alpha$ -Zn grains. Twins observed in the microstructure appeared most likely as a result of the metallographic section preparation. Also, in the case of ZnCu, equiaxed grains of  $\eta$ -Zn were distinguished, suggesting that the alloying additive is fully dissolved in the solid solution. Materials with magnesium addition consist of  $\alpha$ -Zn grains and a eutectic mixture composed of  $\alpha$ -Zn and intermetallic phase  $\text{Mg}_2\text{Zn}_{11}$  located along the Zn grains boundaries. The microstructure of ternary alloy appeared to be similar to Zn-Mg alloy; however, due to Cu addition, it consisted of  $\eta$ -Zn instead of  $\alpha$ -Zn. Based on ImageJ

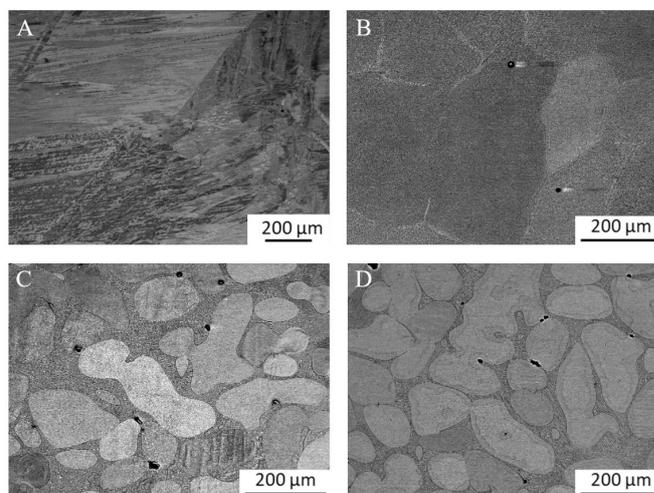


Fig. 2. Microstructures of A) Zn, B) ZnCu, C) ZnMg, D) ZnMgCu obtained in backscattered electron (BSE) mode

The effect of magnesium and copper addition on the microstructure, mechanical properties, and corrosion rate. . .

software, average grain sizes of investigated casts were calculated. Data revealed that alloying additives allowed a significant grain refinement, and that magnesium rather than copper addition contributes best to this (Fig. 3). Pure Zn in the as-cast state has the highest average grain size (approximately 1100  $\mu\text{m}$ ), while the addition of as little Mg as 0.8 wt.% resulted in an almost ten-fold decrease in the average grain size.

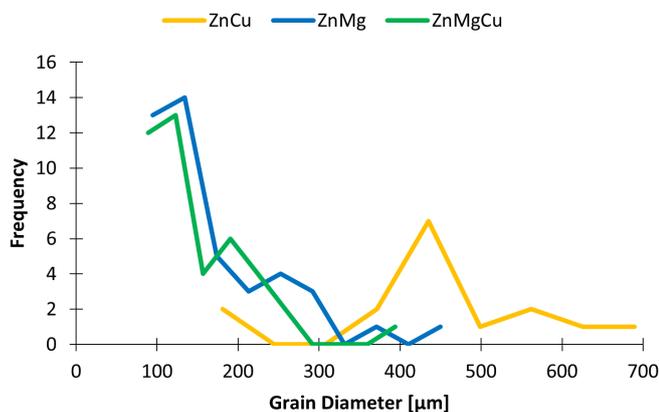


Fig. 3. Grain size distribution of investigated alloys

Further alloying with 0.2 wt.% of Cu, resulting in ternary Zn-MgCu, caused a further decrease, to  $130 \pm 63 \mu\text{m}$ . Additionally, for ZnMg and ZnMgCu alloys, the percentage fraction of the intermetallic  $\text{Mg}_2\text{Zn}_{11}$  phase was calculated. Despite the same amount of Mg addition to alloys, a higher fraction of the phase was calculated for ZnMgCu due to the differences in Zn content in these alloys (99.2 vs 99.0 wt.%, respectively) (Table 1).

Table 1

Average grain size and fraction of intermetallic phase of investigated casts

Material	Average grain size [ $\mu\text{m}$ ]	Fraction of $\text{Mg}_2\text{Zn}_{11}$ [%]
Zn	1100	–
ZnCu	$433 \pm 147$	–
ZnMg	$145 \pm 81$	14
ZnMgCu	$130 \pm 63$	18

With the EDS and XRD techniques, it was possible to carry out qualitative analysis of the chemical composition of alloys. Diffractograms are presented in Fig. 4, and the distribution of the elements through the mapping by EDS in Fig. 5. It was confirmed that, regardless of the material, magnesium was located primarily in the eutectic mixture with negligible amounts dissolved in  $\alpha$ -Zn grains, while copper locates as a solute element both in materials where Cu content is higher, at 1 wt.% in binary ZnCu alloy, and when it is a minor additive of 0.2 wt.% in ternary ZnMgCu, without the formation of any intermetallic phases. For the latter material, the presence of Cu was noticed mainly in the  $\eta$ -Zn matrix and diminished in the area of the intermetallic phase, suggesting its minor solubility.

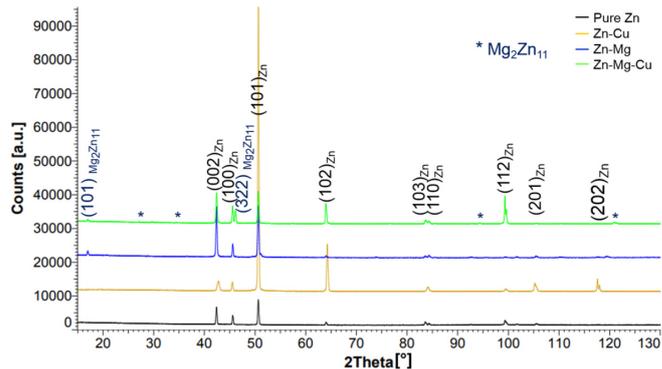


Fig. 4. X-ray diffractograms obtained for analysed materials

### 3.2. Corrosion properties

The two-step corrosion rate investigation was started with electrochemical tests. Table 2 presents the average values of the main parameters obtained from the potentiodynamic test. Corrosion potential ( $E_{\text{corr}}$ ) for Zn and ZnMgCu was at the same level  $-0.943 \text{ V}$ . For binary Zn-based alloys, a significant shift of  $E_{\text{corr}}$  (as compared with pure Zn) was observed for more noble values ( $-0.931 \text{ V}$ ) when copper was added, while for magnesium addition  $E_{\text{corr}}$  decreased to  $-0.970 \text{ V}$ . Those results agree with obtained current density ( $J_{\text{corr}}$ ) and in consequence corrosion rate ( $V_{\text{corr}}$ ).

Table 2


Average values of potentiodynamic test parameters

Material	Corrosion potential [V]	Current density [ $\mu\text{A}/\text{cm}^2$ ]	Corrosion rate [mm/year]
Zn	$-0.943 \pm 0.02$	$20 \pm 2$	$0.36 \pm 0.06$
ZnCu	$-0.931 \pm 0.01$	$18.4 \pm 4$	$0.31 \pm 0.04$
ZnMg	$-0.970 \pm 0.01$	$21.2 \pm 3$	$0.40 \pm 0.08$
ZnMgCu	$-0.943 \pm 0.01$	$20.7 \pm 3$	$0.38 \pm 0.07$

Pure Zn and ternary alloy possessed  $V_{\text{corr}}$  at a similar level (0.36 and 0.38 mm/year, respectively). In the case of ZnCu, compared to pure zinc, a decrease in  $V_{\text{corr}}$  was observed, achieving 0.31 mm/year. The highest degradation rate of 0.4 mm/year was obtained in the case of the ZnMg. The changes in corrosion rate in the function of chemical composition are presented in Fig. 6. It is worth highlighting that the ternary alloy of a composition proposed and designed for the first time in this work has a corrosion rate comparable (within the measurement error) to initial pure Zn material even if any of the additive itself results in significant changes in this property.

To deepen understanding of the alloying element effect on corrosion properties, a static immersion test (IT) was performed. Table 3 presents a summary of the mass of corrosion products, mass loss calculated as a difference between the initial mass of the samples and the weight of the samples after removing corrosion products, and the corrosion rate determined based on mass loss. After 24 h of IT in HBSS, similar results in terms

M. Gieleciak, K. Janus, Ł. Maj, P. Petrzak, M. Bieda, and A. Jarzębska

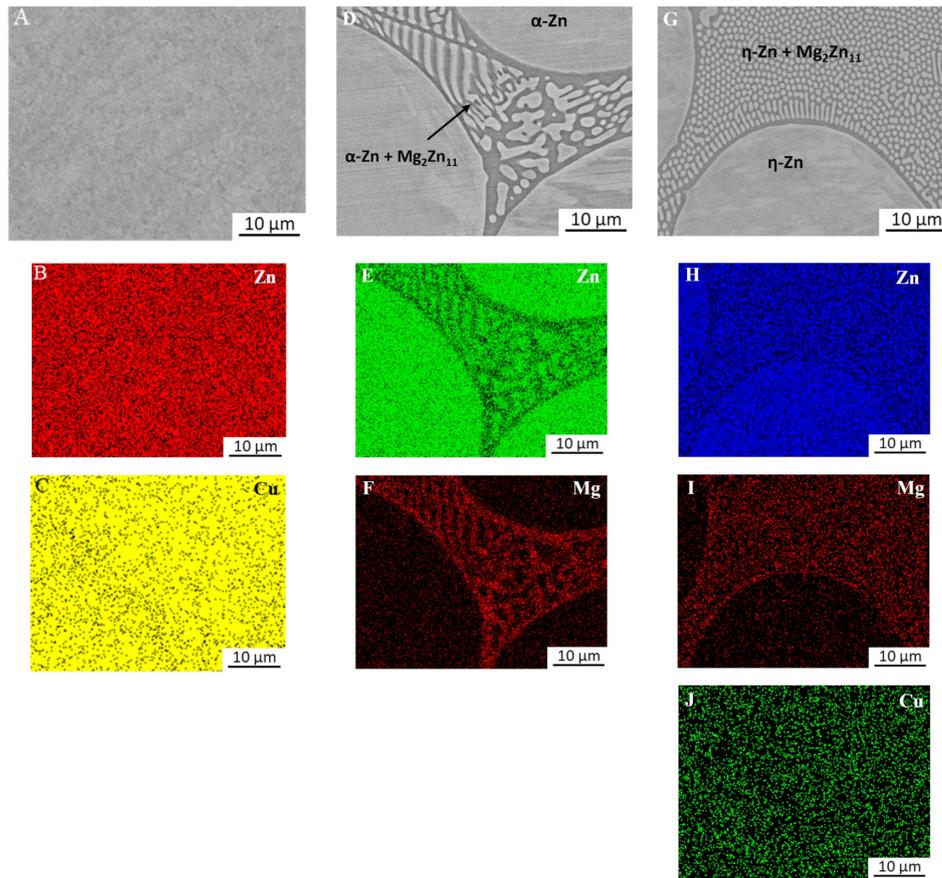

**Fig. 5.** SEM/BSE images of A) ZnCu alloy with distribution maps of B) Zn, C) Cu, D) ZnMg alloy with distribution maps of E) Zn, F) Mg, and G) ZnMgCu alloy with distribution maps of H) Zn, I) Mg and J) Cu

of degradation rate were achieved and stayed in the range of 0.14–0.22 mm/year. However, the tendency of alloys with Cu addition to exhibit higher mass loss and in consequence higher  $V_{corr}$  as compared to pure Zn and the ZnMg alloy was observed for the first 24 h. Prolonged time of immersion (120 h) caused, regardless of chemical composition, a significant decrease in corrosion rate, of about one order of magnitude (Fig. 7). Moreover, after 120 h a rather opposite trend was noticed, as the ternary alloy showed the slowest degradation rate, and pure Zn the fastest. Based on the obtained results, one should conclude the following: for a longer duration of immersion, magnesium inhibits the degradation of Zn-based alloys to a much greater

extent than copper. In all the investigated cases, except the pure Zn, prolonged immersion time resulted in the formation of larger amounts of corrosion products.

SEM observations of sample surfaces exposed to HBSS suggest that after 24 h a discontinuous corrosion products layer was formed. The morphology was similar for each material. Over time, the number of products increased, which correlates with data obtained from mass measurements. After 120 h, a compact layer of corrosion products distributed evenly on the surface was visible in all investigated materials. Examples of the sample surface exposed to HBSS after the different immersion times are given in Fig. 8. After the cleaning procedure of corrosion prod-

**Table 3**

Average values of corrosion products, mass loss, and corrosion rate after static immersion

Material	Mass of corrosion products [mg]		Mass loss [mg]		Corrosion rate [mm/year]	
	24 h	120 h	24 h	120 h	24 h	120 h
Zn	0.29 ± 0.1	0.29 ± 0.2	0.44 ± 0.2	0.99 ± 0.4	0.15 ± 0.05	0.067 ± 0.029
ZnCu	0.27 ± 0.2	0.34 ± 0.1	0.60 ± 0.1	0.80 ± 0.1	0.20 ± 0.01	0.054 ± 0.006
ZnMg	0.24 ± 0.1	0.33 ± 0.1	0.42 ± 0.1	0.67 ± 0.1	0.14 ± 0.02	0.045 ± 0.006
ZnMgCu	0.17 ± 0.1	0.52 ± 0.1	0.64 ± 0.1	0.55 ± 0.1	0.22 ± 0.04	0.038 ± 0.007

The effect of magnesium and copper addition on the microstructure, mechanical properties, and corrosion rate. . .

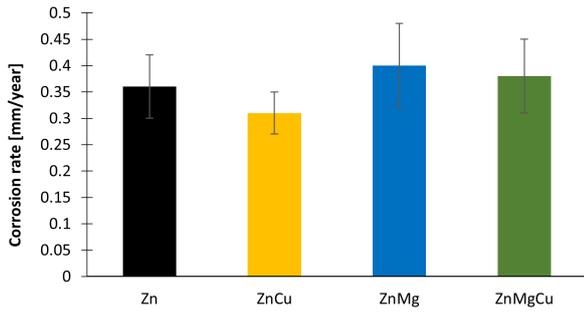


Fig. 6. Corrosion rate determined from electrochemical test

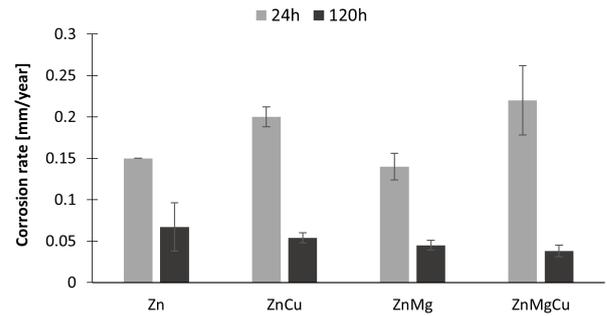


Fig. 7. Corrosion rate determined from static immersion test for 24 h and 120 h


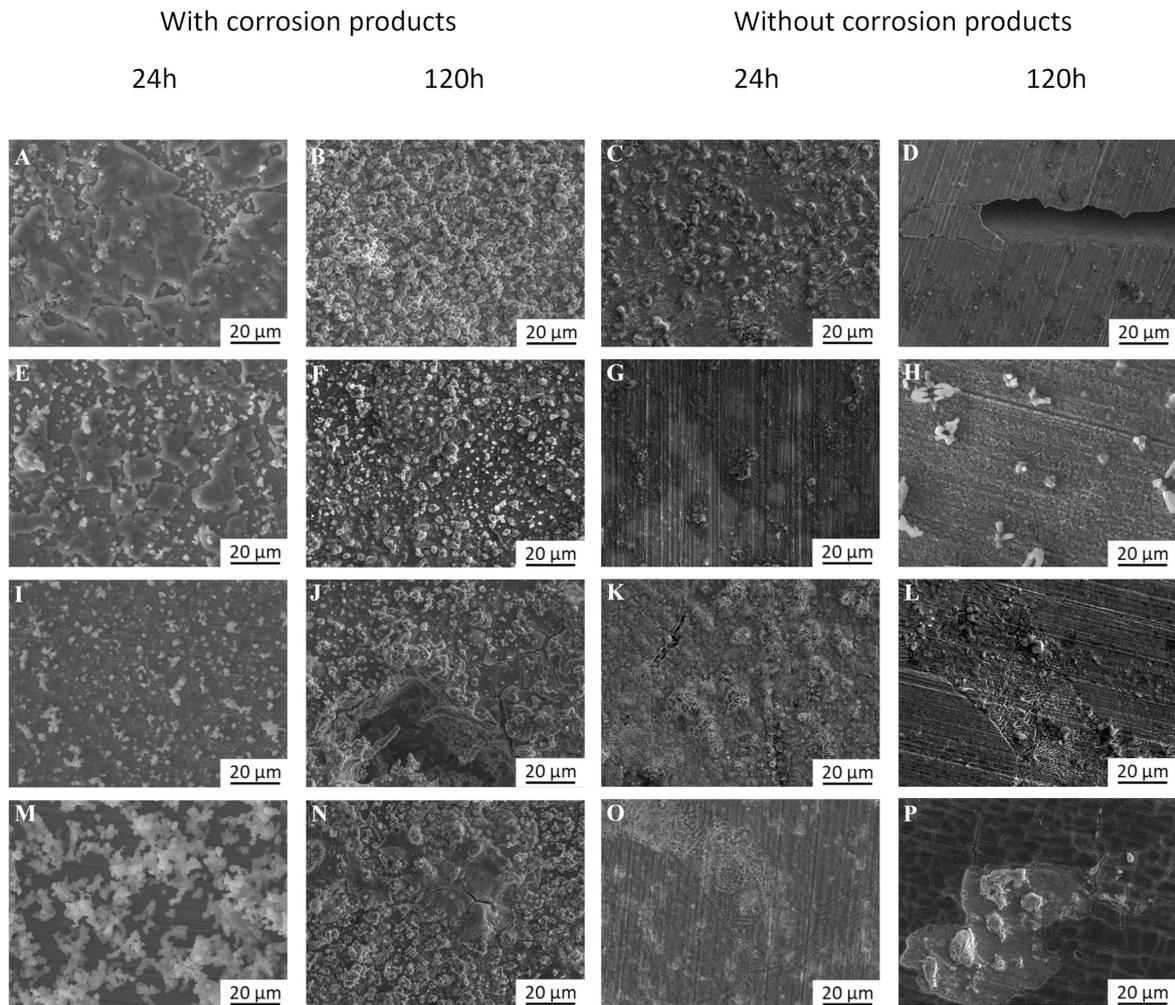


Fig. 8. SEM/SE images samples surface after 24 h and 120 h of immersion test in HBSS and after removing the corrosion products for A–D) pure zinc, E–H) ZnCu, I–L) ZnMg, M–P) ZnMgCu

ucts, SEM images indicate that some of them were still present on the surface. This was especially true for Zn and ZnMg. In two other cases, i.e., ZnCu and ZnMgCu, scratches and single corrosion products were noticeable. For samples after 120 h of IT, products after cleaning were less pronounced and SEM images provided more information.

As regards pure Zn, the presence of large pits and the detachment of substantial portions of the material were observed. In the case of the ZnMg and ZnMgCu, localized corrosion was seen, since in the area of the eutectic mixture an increased number of pits were noticed compared to the grain interior. Moreover, in all investigated cases, the number of pits increased with prolonged

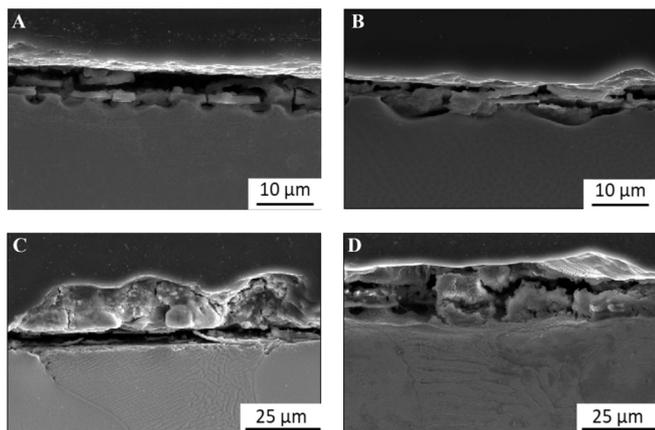


**Fig. 9.** SEM/SE microstructures of corrosion product layer cross-section after 120 h IT of A) pure Zn, B) ZnCu alloy, C) ZnMg alloy and D) ZnMgCu alloy

test duration. The least visible changes compared to the material before immersion were noticed for the ZnCu alloy. Further analysis conducted on cross-sections of the corrosion layer confirmed the calculated corrosion rates. Pure Zn and ZnCu alloys exhibited more developed surfaces with numerous pits compared to the alloys containing Mg (Fig. 9). This complied with measured mass loss, where 0.99 and 0.80 mg weight decrease was achieved for pure Zn and ZnCu alloy, respectively, which was higher by at least 13 mg than in the case of Mg-contented alloys. Moreover, it was noticed that alloying additives lead to an increase in the corrosion layer thickness, compared to pure Zn. This effect was more pronounced in the case of Mg addition rather than Cu. The thick, dense layer of corrosion products was especially visible near the intermetallic phase. SEM observations were supported by measuring the average thickness of the corrosion layer using ImageJ (see Table 4). Chemical composition investigation from cross-sections of the corrosion product layer, after 120 h of IT was performed using the EDS technique. This revealed that there was no significant difference in the chemical composition of the layer of corrosion products, regardless of alloying additives. In the majority, apart from Zn and alloying additives, the corrosion products layer consisted of oxygen (O), chlorine (Cl), calcium (Ca), and phosphorus (P). It was noticed that Cl and Mg tend to be located in some specific places, while Zn, O, Ca and P were distributed evenly in whole volume of the layer. The example of distribution of particular elements within the corrosion product layer is presented in Fig. 10.

**Table 4**

Average corrosion layer thickness

Material	Average corrosion layer thickness [ $\mu\text{m}$ ]
Zn	$6 \pm 1$
ZnCu	$5.5 \pm 1$
ZnMg	$20 \pm 4$
ZnMgCu	$22 \pm 3$

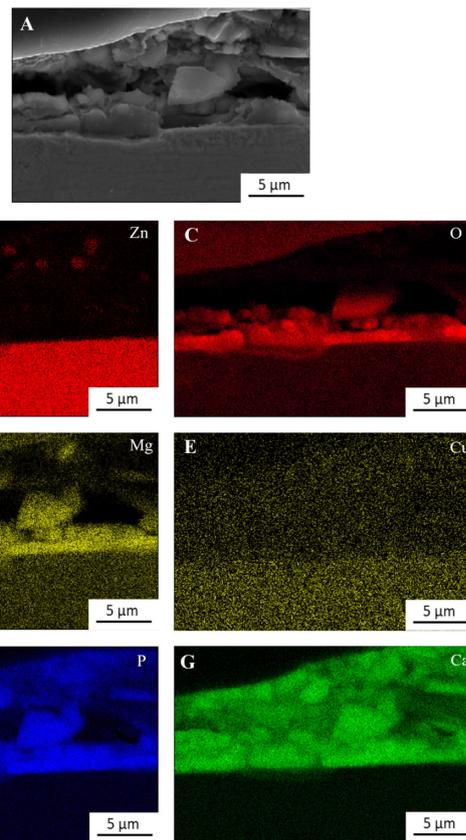

**Fig. 10.** SEM/SE microstructures of corrosion product layer cross-section after 120 h IT of ZnMgCu alloy A) with corresponding distribution of B) Zn, C) O, D) Mg, E) Cu, F) P and G) Ca

### 3.3. Mechanical properties

To establish how alloying additives affect the mechanical properties of the Zn material, a static tensile test was performed. Based on stress-strain curves, presented in Fig. 9, average values of yield strength (YS), ultimate tensile strength (UTS), and elongation (A) were determined and listed (Table 5). In reference to [18], it was confirmed that pure Zn possesses very low mechanical strength expressed in YS and UTS of 10 MPa and 18 MPa, respectively, with elongation as low as 0.3%. Alloying Zn with low magnesium and/or copper content significantly increases not only mechanical strength but also elongation. Based on the results, one may conclude that the best combination of strength and elongation was obtained for the ZnMgCu, for

**Table 5**

Average mechanical property values for the investigated materials

Material	YS [MPa]	UTS [MPa]	A [%]
Zn*	10	18	0.3
ZnCu	$37 \pm 5$	$69 \pm 5$	$4.5 \pm 0.7$
ZnMg	$53 \pm 7$	$70 \pm 8$	$1.4 \pm 0.2$
ZnMgCu	$54 \pm 4$	$81 \pm 4$	$1.6 \pm 0.7$

\* Results from the literature [18]

which YS and UTS were as high as 54 MPa and 81 MPa, respectively, with A of 1.6%. The character of the stress-strain curves (Fig. 11) for alloys with Mg addition indicated the brittleness of the materials, while ZnCu was more ductile.

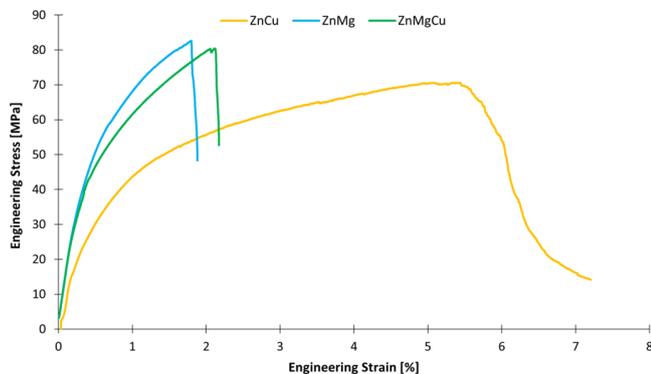


Fig. 11. Representative stress-strain curves from static tensile test

Similar properties were also observed during the microstructure analysis of tensile-tested samples. Optical microscopy observation of the surface of dog-bone samples confirmed the brittle fracture in alloys with magnesium addition. The zinc phase tends to deform, and brittle cracking occurs in regions where a eutectic mixture is present. In the case of ZnCu, the occurrence of twins was noticed on the surface, especially close to the cracked site (Fig. 12). Moreover, SEM/SE observations of the fractures correspond well with other results, since an almost flat surface was observed in the case of ZnMg and ZnMgCu alloys, suggesting brittle fracture. Meanwhile, for ZnCu, a more developed surface with visible voids indicates plasticity.


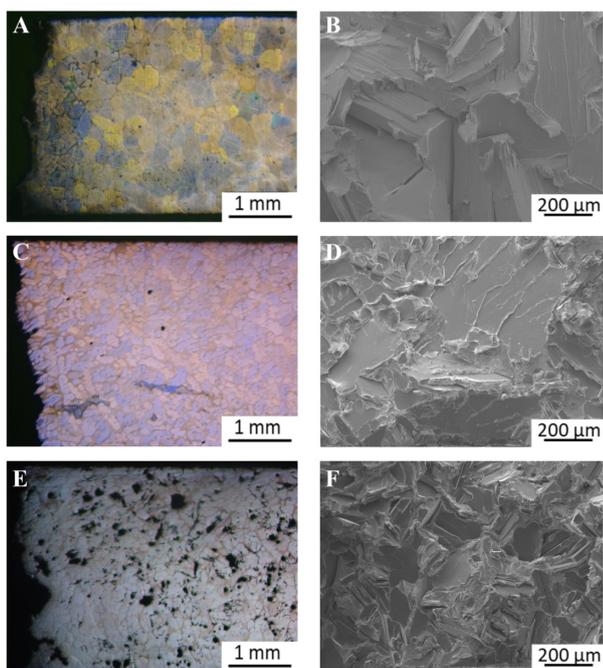


Fig. 12. Microstructure of A) ZnCu, C) ZnMg, E) ZnMgCu alloy after static tensile test and corresponding B), D), F) SEM/SE fractures

#### 4. DISCUSSION

In this work, pure zinc, as a reference material, and three alloys (ZnCu, ZnMg, and ZnMgCu) in an as-cast state were characterized. Microstructural analysis indicated an effect of alloying additives, especially magnesium, on grain refinement. This is confirmed by the average grain size determination, which for pure zinc was over 1000  $\mu\text{m}$ , for ZnCu about 430  $\mu\text{m}$ , and for magnesium close to 150  $\mu\text{m}$ . Based on the binary equilibrium phase diagrams of Zn-Mg one, it should be noted that the addition of Mg even as low as 0.1 wt.% results in the formation of an  $\text{Mg}_2\text{Zn}_{11}$  intermetallic phase [9]. The volume fraction of  $\text{Mg}_2\text{Zn}_{11}$  of 14%, calculated in this work, forming the eutectic mixture, significantly inhibited grain growth during the casting process [9, 13]. This allows one to assume that to obtain a fine-grained microstructure, it is more advantageous to select chemical elements that form with zinc-based second phases [19]. In this way, the effect of Cu in the microstructure refinement is much less pronounced even with the addition of 1 wt.%, which did not allow intermetallic phases to form (the maximum solubility of Cu in  $\eta$ -Zn is 2.7 wt.% according to the phase diagram [19]), and all the copper is substituted for the Zn atoms in its crystal structure. For ternary ZnMgCu alloy, the eutectic mixture ( $\eta$ -Zn+ $\text{Mg}_2\text{Zn}_{11}$ ), formed at the grain boundaries of Zn grains, inhibits grain growth more efficiently than Cu dissolved in the Zn grains. Thus, the changes in the average grain size and resulting mechanical properties between ZnMg and ZnMgCu are negligible. Similar results can be observed in the literature [17, 20–24]. Based on the results of the electrochemical test, it can be concluded that the addition of copper increases the corrosion resistance of zinc, while magnesium causes its decrease. According to the electrochemical series copper has +0.34 V and zinc -0.76 V, so Cu improves corrosion properties, while magnesium (-2.37 V) contributes to faster degradation [25, 26]. For this reason, the addition of copper to ZnMg led to a reduction in the corrosion rate value. However, this was not in correlation with the results obtained from the immersion test, where the list from last to most corrosion resistant was as follows: for 24 h ZnMgCu > ZnCu > Zn > ZnMg and for 120 h Zn > ZnCu > ZnMg > ZnMgCu. It should be underlined that, in the case of 24 h IT, the degradation rate values were very similar. However, the discrepancy between the corrosion rate assessed based on electrochemical and immersion tests is not unusual and has already been found in the literature [27]. It is more reasonable to determine corrosion rate based on immersion testing because it is prolonged in time and closer to behaviour in the physiological environment. Moreover, the process is not forced by the polarization of the sample. Results indicate that the grain size seems to be a crucial factor affecting corrosion rate [13]. Results from the static immersion test performed for 120 h showed a clear correlation between grain size and corrosion rate (Fig. 13). Similar results were found in the literature [28, 29], where a decrease in the  $V_{\text{corr}}$  was also noted for zinc-magnesium and zinc-copper alloys. Furthermore, ternary zinc alloy was characterized by the thickest corrosion products layer and the lowest mass loss after 120 h IT. A thicker layer of corrosion products was observed in the vicinity of the eutectic

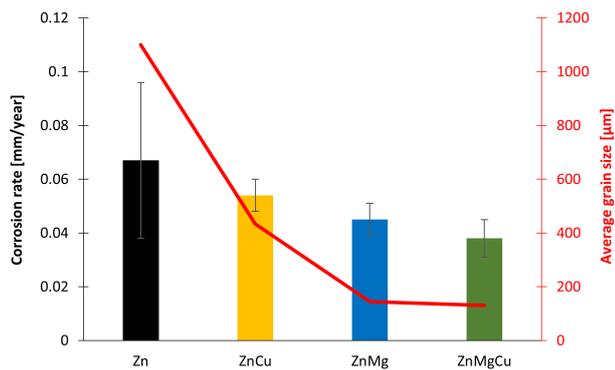

**Fig. 13.** Relation between grain size and corrosion rate calculated based on mass loss of the samples exposed to HBSS for 120 h

mixture, which can be explained by the fact that magnesium ions are also released into the corrosive solution, thus facilitating the formation of subsequent products [30]. This was also confirmed by SEM observations of corrosion products. After removing the corrosion products in the ZnMgCu alloy, the eutectic mixture was exposed, which implies that it is a specific place for degradation. A more compact layer of products can protect the material from degradation, which contributes to lowering the corrosion rate of the ZnMgCu alloy. Moreover, this phenomenon can be intensified by the increased number of grain boundaries in Zn-MgCu alloys. In general, grain boundaries are more reactive than grain interior, thus facilitating ion transport and the creation of a protective layer [31]. Alloying additives affect mechanical properties in different ways, depending on the chemical composition. They can strengthen zinc by the formation of a eutectic mixture (ZnMg and ZnMgCu) or by a solid solution (ZnCu, ZnMgCu). Both of these elements affect the grain growth during casting (microstructure refinement as compared with pure Zn). What is more, all these microstructure features constitute an obstacle to the movement of dislocations during the tensile test increasing the mechanical strength. In summary, the ZnMgCu alloy with the contribution of all of the mentioned strengthening mechanisms, described by the smallest grain size, with the presence of eutectic mixture and Cu dissolved in the solution, results in the best YS and UTS for this material. The low elongation of materials with the addition of Mg is a consequence of the presence of the brittle  $Mg_2Zn_{11}$  phase. However, alloying zinc with Cu increases elongation during tensile testing. Several hypotheses have been developed to explain this effect, of which the main, proposing the occurrence of twinning during deformation, is the most common [10, 12, 14, 16, 17, 21].

## 5. CONCLUSIONS

Results lead to the following conclusions:

1. Alloying additives contribute to decreasing average grain size. The most favourable effect was achieved by the addition of magnesium, which formed a eutectic mixture located at  $\alpha$ -Zn grains preventing grain growth during casting. The addition of copper has a less pronounced effect on the mi-

crostructure refinement, as all its atoms dissolved in the  $\eta$ -Zn grain structure.

2. The results of potentiodynamic corrosion tests suggest that the ternary ZnMgCu alloy, with a composition proposed and designed for the first time in this work, has a corrosion rate comparable to the initial pure Zn material, even if any of the additive itself results in significant changes in this property.
3. Immersing the samples in HBSS solution gave more complex results as the tendencies depend on whether the samples were investigated for 24 or 120 h. A longer immersion test resulted in far lower corrosion rates compared with the first 24 h. Moreover, for 120 h a relation between corrosion rate and grain size was noticed. The smaller the grain size, the more corrosion-resistant the material was.
4. Increased number of alloying elements affected the formation of the corrosion product layer. The thickest layer was observed for ZnMgCu, which was connected with the  $Mg_2Zn_{11}$  phase and grain refinement.
5. ZnMgCu possessed the highest mechanical strength due to the presence of magnesium facilitating the formation of the eutectic mixture (with the presence of a hard but brittle  $Mg_2Zn_{11}$  intermetallic phase) allowing significant refinement of the microstructure and copper being dissolved within the refined  $\eta$ -Zn grains.
6. Results indicate the effect of a particular element on microstructure as well as on mechanical and corrosion properties. Detailed characterization of the materials in an as-cast state established the unambiguous impact of alloying, which may contribute to the selection of potential material for further research in the context of applications as biodegradable stents. From our results, it seems that ternary ZnMgCu is the most promising one.

## ACKNOWLEDGEMENTS

This work was supported by the National Centre for Research and Development, grant number LIDER/54/0229/L-11/19/NCBR/2020.

## REFERENCES

- [1] X. Tong *et al.*, "Biodegradable Zn-Cu-Li alloys with ultra-high strength, ductility, antibacterial ability, cytocompatibility, and suitable degradation rate for potential bone-implant applications," *Smart Mater. Manuf.*, vol. 1, p. 100012, 2023, doi: [10.1016/j.smmf.2022.100012](https://doi.org/10.1016/j.smmf.2022.100012).
- [2] X. Liu *et al.*, "Micro-alloying with Mn in Zn-Mg alloy for future biodegradable metals application," *Mater. Des.*, vol. 94, pp. 95–104, Mar. 2016, doi: [10.1016/j.matdes.2015.12.128](https://doi.org/10.1016/j.matdes.2015.12.128).
- [3] H. Gong, K. Wang, R. Strich, and J.G. Zhou, "In vitro biodegradation behavior, mechanical properties, and cytotoxicity of biodegradable Zn-Mg alloy," *J. Biomed. Mater. Res. B Appl. Biomater.*, vol. 103, no. 8, pp. 1632–1640, Nov. 2015, doi: [10.1002/jbm.b.33341](https://doi.org/10.1002/jbm.b.33341).
- [4] P.K. Bowen, J. Drelich, and J. Goldman, "Zinc Exhibits Ideal Physiological Corrosion Behavior for Bioabsorbable Stents," *Adv. Mater.*, vol. 25, no. 18, pp. 2577–2582, May 2013, doi: [10.1002/adma.201300226](https://doi.org/10.1002/adma.201300226).

- [5] P.K. Bowen *et al.*, “Biodegradable Metals for Cardiovascular Stents: from Clinical Concerns to Recent Zn-Alloys,” *Adv. Healthc. Mater.*, vol. 5, no. 10, pp. 1121–1140, May 2016, doi: [10.1002/adhm.201501019](https://doi.org/10.1002/adhm.201501019).
- [6] L. Kong, Z. Heydari, G.H. Lami, A. Saberi, M.S. Baltatu, and P. Vizureanu, “A Comprehensive Review of the Current Research Status of Biodegradable Zinc Alloys and Composites for Biomedical Applications,” *Materials*, vol. 16, no. 13, p. 4797, Jul. 2023, doi: [10.3390/ma16134797](https://doi.org/10.3390/ma16134797).
- [7] E. Mostaed, M. Sikora-Jasinska, J.W. Drelich, and M. Vedani, “Zinc-based alloys for degradable vascular stent applications,” *Acta Biomater.*, vol. 71, pp. 1–23, Apr. 2018, doi: [10.1016/j.actbio.2018.03.005](https://doi.org/10.1016/j.actbio.2018.03.005).
- [8] H. Kabir, K. Munir, C. Wen, and Y. Li, “Recent research and progress of biodegradable zinc alloys and composites for biomedical applications: Biomechanical and biocorrosion perspectives,” *Bioact. Mater.*, vol. 6, no. 3, pp. 836–879, Mar. 2021, doi: [10.1016/j.bioactmat.2020.09.013](https://doi.org/10.1016/j.bioactmat.2020.09.013).
- [9] S. Liu, D. Kent, N. Doan, M. Dargusch, and G. Wang, “Effects of deformation twinning on the mechanical properties of biodegradable Zn–Mg alloys,” *Bioact. Mater.*, vol. 4, pp. 8–16, Dec. 2019, doi: [10.1016/j.bioactmat.2018.11.001](https://doi.org/10.1016/j.bioactmat.2018.11.001).
- [10] C. Shen *et al.*, “Mechanical properties, in vitro degradation behavior, hemocompatibility and cytotoxicity evaluation of Zn–1.2 Mg alloy for biodegradable implants,” *RSC Adv.*, vol. 6, no. 89, pp. 86410–86419, 2016, doi: [10.1039/C6RA14300H](https://doi.org/10.1039/C6RA14300H).
- [11] J. Kubásek, D. Vojtěch, I. Pospíšilová, A. Michalcová, and J. Maixner, “Microstructure and mechanical properties of the micrograined hypoeutectic Zn–Mg alloy,” *Int. J. Miner. Metall. Mater.*, vol. 23, no. 10, pp. 1167–1176, Oct. 2016, doi: [10.1007/s12613-016-1336-7](https://doi.org/10.1007/s12613-016-1336-7).
- [12] M.S. Dambatta, S. Izman, D. Kurniawan, and H. Hermawan, “Processing of Zn–3Mg alloy by equal channel angular pressing for biodegradable metal implants,” *J. King Saud. Univ. Sci.*, vol. 29, no. 4, pp. 455–461, Oct. 2017, doi: [10.1016/j.jksus.2017.07.008](https://doi.org/10.1016/j.jksus.2017.07.008).
- [13] L. Ye *et al.*, “Effect of grain size and volume fraction of eutectic structure on mechanical properties and corrosion behavior of as-cast Zn–Mg binary alloys,” *J. Mater. Res. Technol.*, vol. 16, pp. 1673–1685, Jan. 2022, doi: [10.1016/j.jmrt.2021.12.101](https://doi.org/10.1016/j.jmrt.2021.12.101).
- [14] P. Li *et al.*, “Investigation of zincopper alloys as potential materials for craniomaxillofacial osteosynthesis implants,” *Mater. Sci. Eng.-C*, vol. 103, p. 109826, Oct. 2019, doi: [10.1016/j.msec.2019.109826](https://doi.org/10.1016/j.msec.2019.109826).
- [15] X. Liu *et al.*, “Microstructure, mechanical properties, in vitro degradation behavior and hemocompatibility of novel Zn–Mg–Sr alloys as biodegradable metals,” *Mater. Lett.*, vol. 162, pp. 242–245, Jan. 2016, doi: [10.1016/j.matlet.2015.07.151](https://doi.org/10.1016/j.matlet.2015.07.151).
- [16] L. Zhang, X.Y. Liu, H. Huang, and W. Zhan, “Effects of Ti on microstructure, mechanical properties and biodegradation behavior of Zn–Cu alloy,” *Mater. Lett.*, vol. 244, pp. 119–122, Jun. 2019, doi: [10.1016/j.matlet.2019.02.071](https://doi.org/10.1016/j.matlet.2019.02.071).
- [17] X. Liu *et al.*, “Effects of alloying elements (Ca and Sr) on microstructure, mechanical property and in vitro corrosion behavior of biodegradable Zn–1.5Mg alloy,” *J. Alloys Compd.*, vol. 664, pp. 444–452, Apr. 2016, doi: [10.1016/j.jallcom.2015.10.116](https://doi.org/10.1016/j.jallcom.2015.10.116).
- [18] H.F. Li *et al.*, “Development of biodegradable Zn–1X binary alloys with nutrient alloying elements Mg, Ca and Sr,” *Sci. Rep.*, vol. 5, no. 1, p. 12190, Aug. 2015, doi: [10.1038/srep12190](https://doi.org/10.1038/srep12190).
- [19] J. Lin *et al.*, “Biodegradable Zn–3Cu and Zn–3Cu–0.2Ti alloys with ultrahigh ductility and antibacterial ability for orthopedic applications,” *J. Mater. Sci. Technol.*, vol. 68, pp. 76–90, Mar. 2021, doi: [10.1016/j.jmst.2020.06.052](https://doi.org/10.1016/j.jmst.2020.06.052).
- [20] M. Wątroba *et al.*, “Design of novel Zn–Ag–Zr alloy with enhanced strength as a potential biodegradable implant material,” *Mater. Des.*, vol. 183, p. 108154, Dec. 2019, doi: [10.1016/j.matdes.2019.108154](https://doi.org/10.1016/j.matdes.2019.108154).
- [21] X. Wang, Y. Ma, B. Meng, and M. Wan, “Effect of equal-channel angular pressing on microstructural evolution, mechanical property and biodegradability of an ultrafine-grained zinc alloy,” *Mater. Sci. Eng.-A*, vol. 824, p. 141857, Sep. 2021, doi: [10.1016/j.msea.2021.141857](https://doi.org/10.1016/j.msea.2021.141857).
- [22] L. Li *et al.*, “Investigation on microstructures, mechanical properties and in vitro corrosion behavior of novel biodegradable Zn–2Cu–0.01Ti–xLi alloys,” *J. Alloys Compd.*, vol. 888, p. 161529, Dec. 2021, doi: [10.1016/j.jallcom.2021.161529](https://doi.org/10.1016/j.jallcom.2021.161529).
- [23] X. Tong *et al.*, “Development of biodegradable Zn–1Mg–0.1RE (RE = Er, Dy, and Ho) alloys for biomedical applications,” *Acta Biomater.*, vol. 117, pp. 384–399, Nov. 2020, doi: [10.1016/j.actbio.2020.09.036](https://doi.org/10.1016/j.actbio.2020.09.036).
- [24] J. Lin *et al.*, “Biodegradable ternary Zn–3Ge–0.5X (X=Cu, Mg, and Fe) alloys for orthopedic applications,” *Acta Biomater.*, vol. 115, pp. 432–446, Oct. 2020, doi: [10.1016/j.actbio.2020.08.033](https://doi.org/10.1016/j.actbio.2020.08.033).
- [25] G. Katarivas Levy, J. Goldman, and E. Aghion, “The Prospects of Zinc as a Structural Material for Biodegradable Implants—A Review Paper,” *Metals (Basel)*, vol. 7, no. 10, p. 402, Oct. 2017, doi: [10.3390/met7100402](https://doi.org/10.3390/met7100402).
- [26] S. Huang, L. Wang, Y. Zheng, L. Qiao, and Y. Yan, “In vitro degradation behavior of novel Zn–Cu–Li alloys: Roles of alloy composition and rolling processing,” *Mater. Des.*, vol. 212, p. 110288, Dec. 2021, doi: [10.1016/j.matdes.2021.110288](https://doi.org/10.1016/j.matdes.2021.110288).
- [27] C. García-Mintegui *et al.*, “Zn–Mg and Zn–Cu alloys for stenting applications: From nanoscale mechanical characterization to in vitro degradation and biocompatibility,” *Bioact. Mater.*, vol. 6, no. 12, pp. 4430–4446, Dec. 2021, doi: [10.1016/j.bioactmat.2021.04.015](https://doi.org/10.1016/j.bioactmat.2021.04.015).
- [28] G. Bao *et al.*, “Feasibility evaluation of a Zn–Cu alloy for intrauterine devices: In vitro and in vivo studies,” *Acta Biomater.*, vol. 142, pp. 374–387, Apr. 2022, doi: [10.1016/j.actbio.2022.01.053](https://doi.org/10.1016/j.actbio.2022.01.053).
- [29] J. Huang *et al.*, “Preparation and Properties of Zn–Cu Alloy for Potential Stent Material,” *J. Mater. Eng. Perform.*, vol. 29, no. 10, pp. 6484–6493, Oct. 2020, doi: [10.1007/s11665-020-05167-0](https://doi.org/10.1007/s11665-020-05167-0).
- [30] M.M. Alves, T. Prošek, C.F. Santos, and M.F. Montemor, “Evolution of the in vitro degradation of Zn–Mg alloys under simulated physiological conditions,” *RSC Adv.*, vol. 7, no. 45, pp. 28224–28233, 2017, doi: [10.1039/C6RA28542B](https://doi.org/10.1039/C6RA28542B).
- [31] K.D. Ralston and N. Birbilis, “Effect of Grain Size on Corrosion: A Review,” *Corrosion*, vol. 66, no. 7, pp. 075005–075005–13, Jul. 2010, doi: [10.5006/1.3462912](https://doi.org/10.5006/1.3462912).